



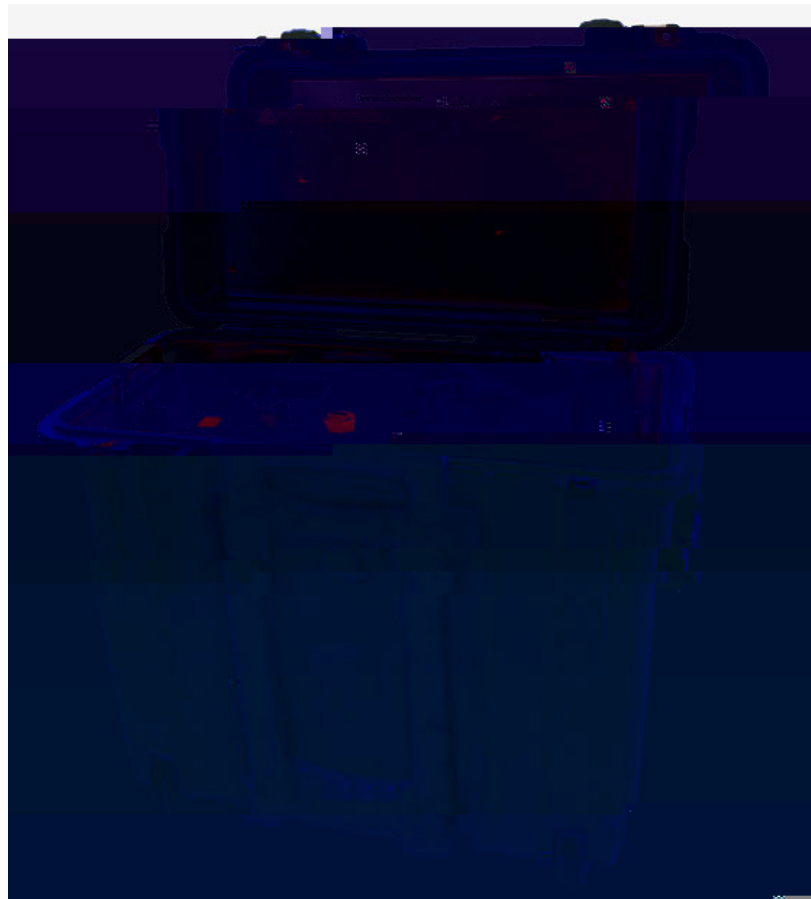

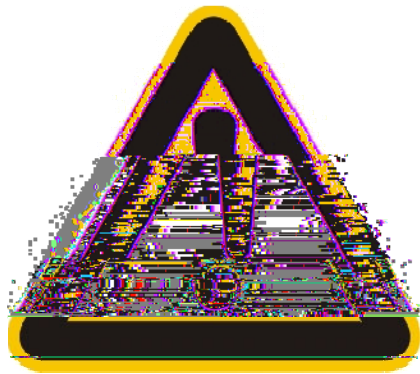

1		4
1.1		4
1.2		4
1.3		5
2		5
3		6
3.1		6
3.2		7
3.3		7
3.3.1		7

4.....ù

¶.1 ù

¶.2.....ê.....

ê.....

ê

/

,

1.3

0 60kV

500mA

0 4kV

500mA

4. 10A 5 × 20

5. 220V ± 10%

6.



7.


3.2

3.3

3.3

3.3.1

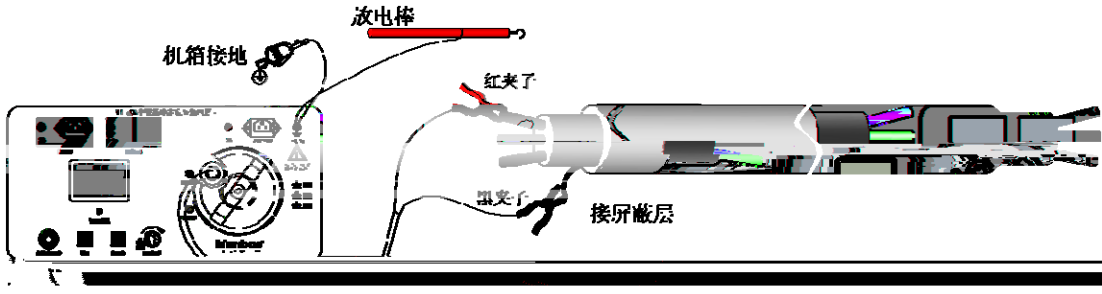	 2	
1		
2		
	 高压分	
	 高压合	  



4.2

1

2

3

1

2

3


1

2

3

4.3

4.3.1

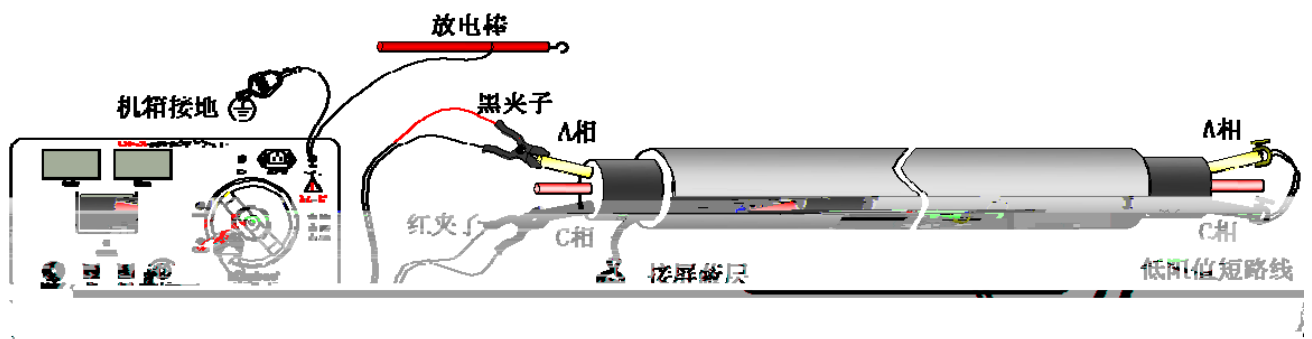

1.


2.

3. FJ2

4.


4.3.2

4.3.2.1 /



/



4 /



4.3.2.2


1.



	 高压分	

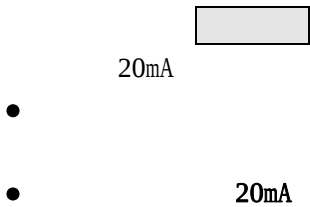	 高压合	
	 零位启动 高压调节	 20mA 20mA

2.

/

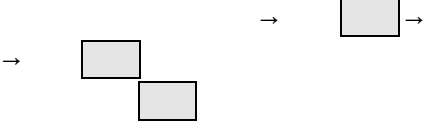	 电桥法 截面法 电压法 设置	
	 电桥法 设置电缆长度 00100m 启动 退出	

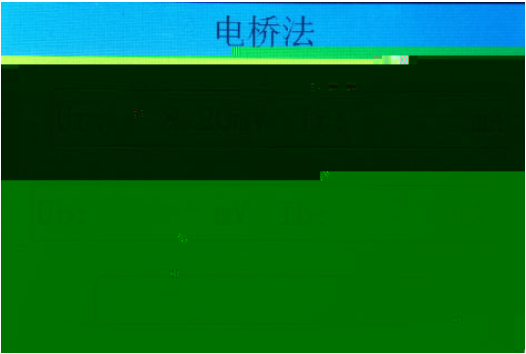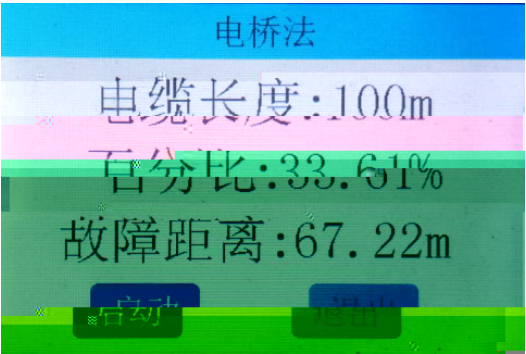		● “4. ”
		□
	→ □ →	0 → □ →

●

3. □ / □

		□

	截面法 截面积:025mm² 材质:铝 启动退出	→ →
	截面法	“4.”
	截面法 材质:铝 截面积:025mm² 启动退出	
	→ →	0→ →

●

4

	20mA	“4”

4.4




- 1 :
- 2 :

7.1

4.4.1

1.

	5 + 1 2 FJ3 3
	4.4 “ 4.4.2.2 ”


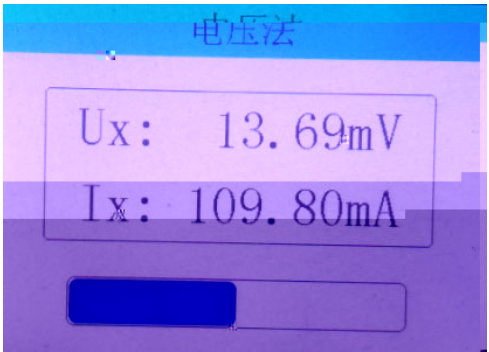
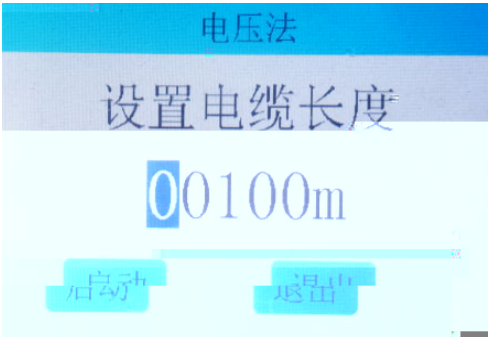


•

•

”

4.4.2.2 “4.

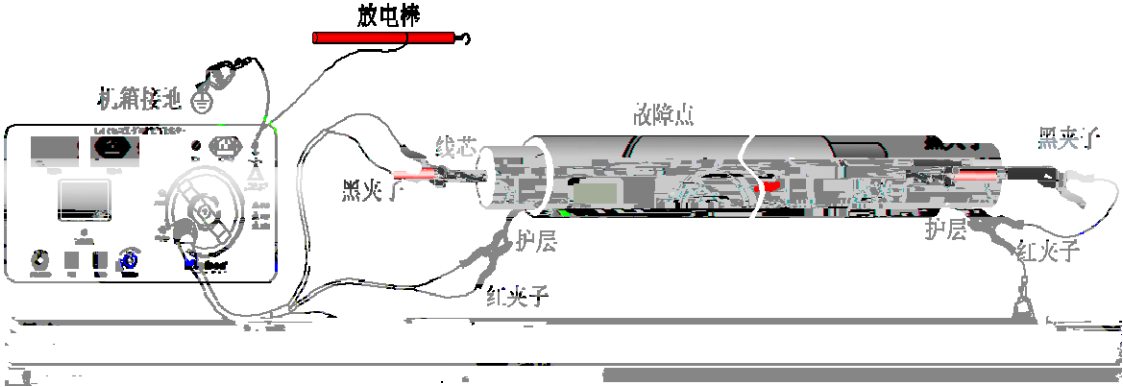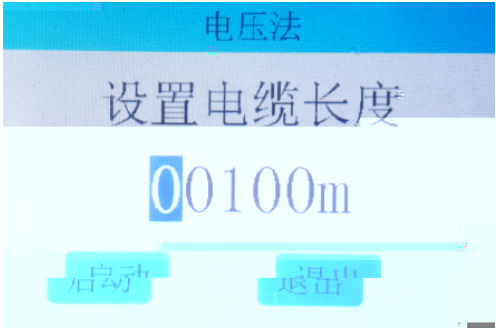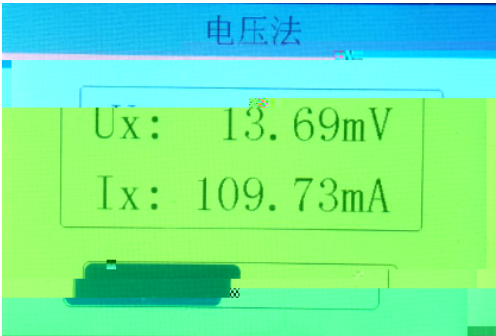	 6 + 1 2	
	3.4 “3.4.2.2”	
		
		
		4.4.2.2 “4.”

	电压法 电缆长度:100m 百分比:94.75% 故障距离:94.75m 启动	
	→ 0→ →	

5

1.

2. 60kV

3.1

3.

4.

5.

3.3.2

5

6.


7.

8.


6

6.1

6.1.1

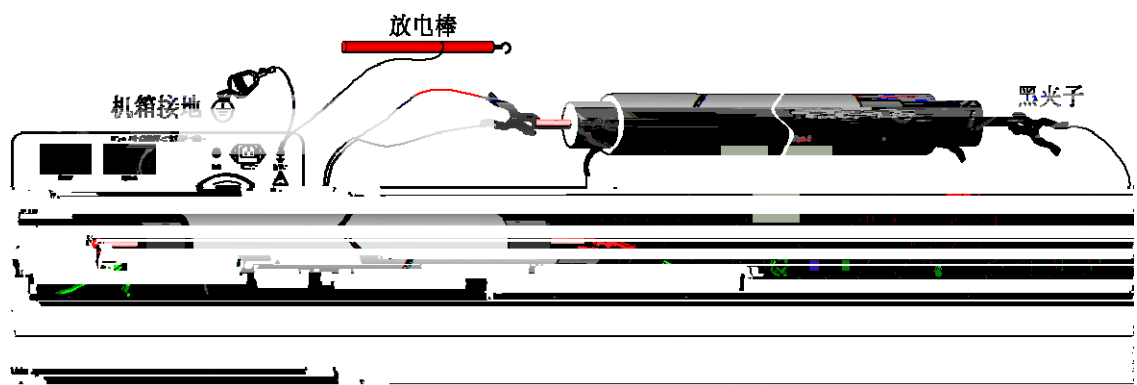


1

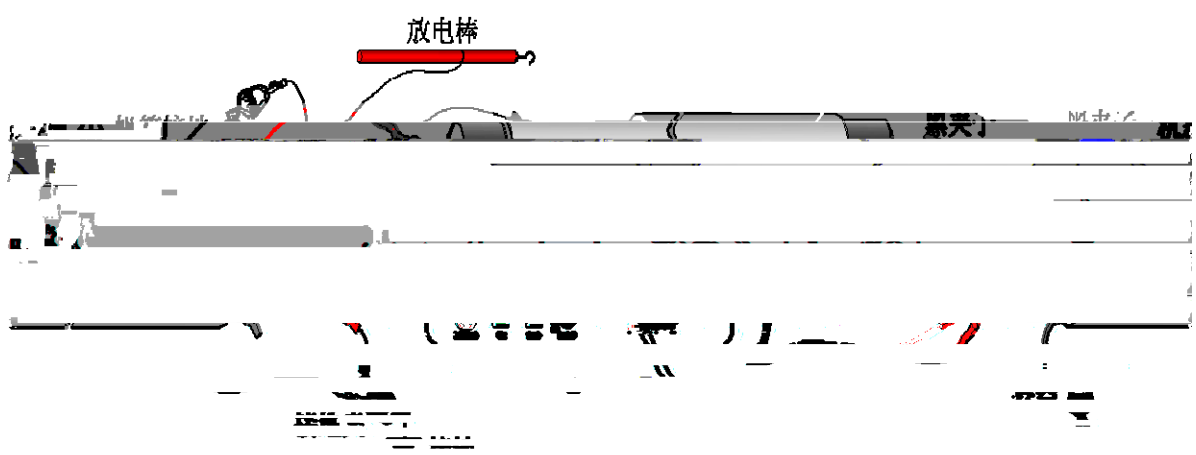


2

6.1.2

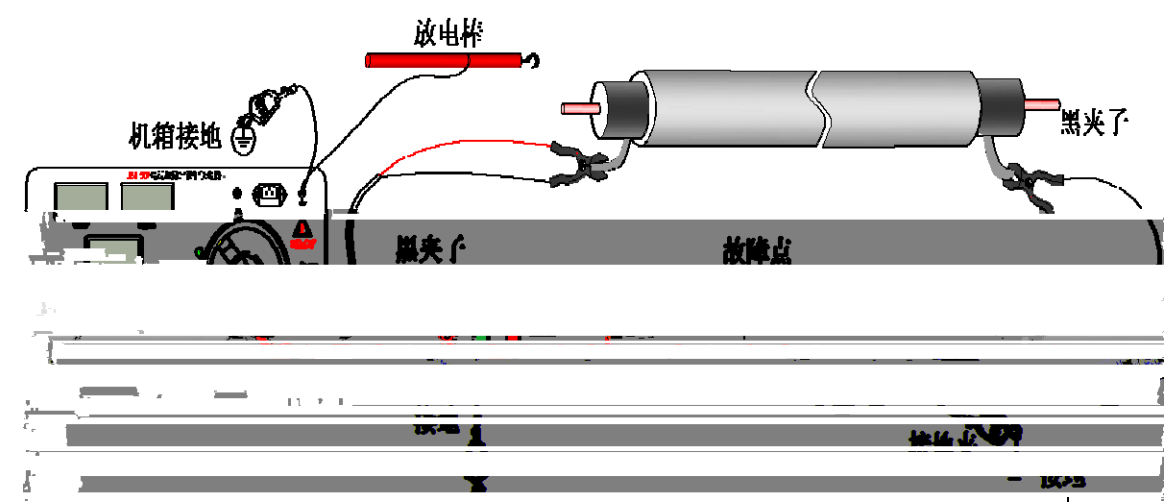

3

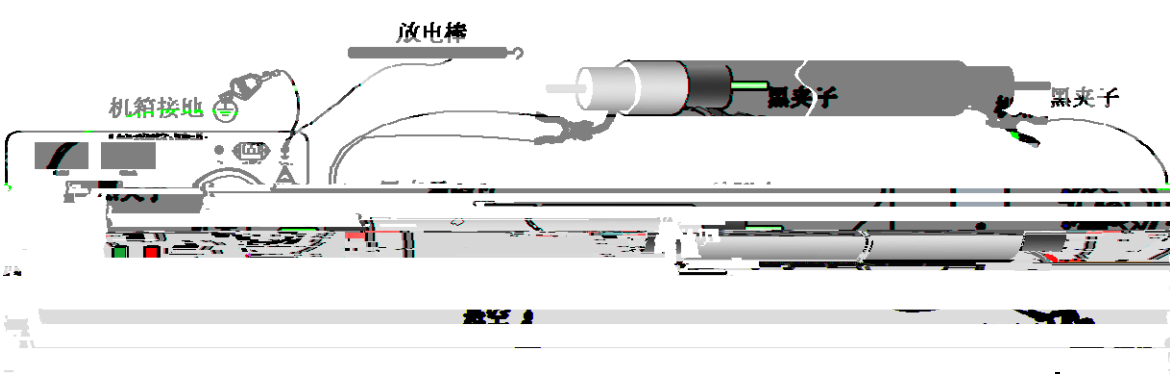

4

3 4


6.2





5

33.3%

6.3

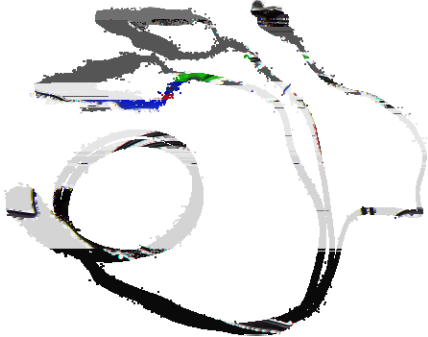1		FJ1 3.5) FJ1L 20)	((
2		FJ2	
3		FJ3 FJ3L 10	4

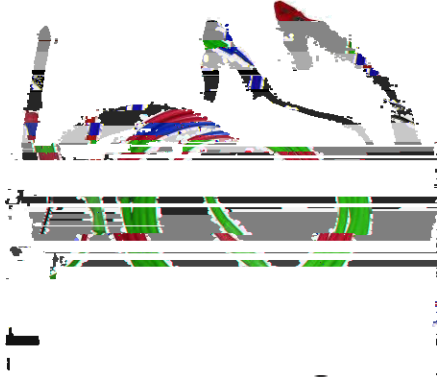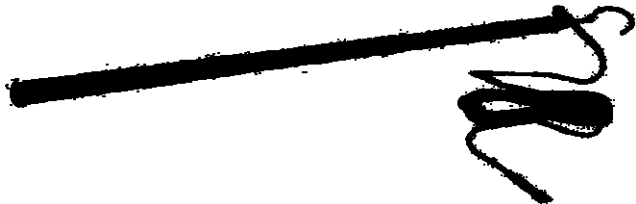4		FJ4 FJ4L)	(3.5) (20
5			
6	