
OPERATION MANUAL

CT2679C

2 15

310017

0571-89935600

0571-89935608

E-MAIL hzhv@hzhv.com

www.hzhv.com

		4
1.1		4
1.2		4
1.2		5
		6
		7
3.1		7
3.2		8
3.3		8
		9
4.1		9
4.2		9
4.3		12
4.4		14
4.5	m " è	

1.1

“ ”

1.2

- 0 5000V (100V)
- 0.01uF
- 0.1uS
- <5%(1kV 5kV)
- 320 * 240
- 50W
- AC220V ± 10%, 50Hz
- 0 40
- ≤ 85%
- 380 × 340 × 130 mm × ×
- 8Kg

1.3

Q

RLC

1-1

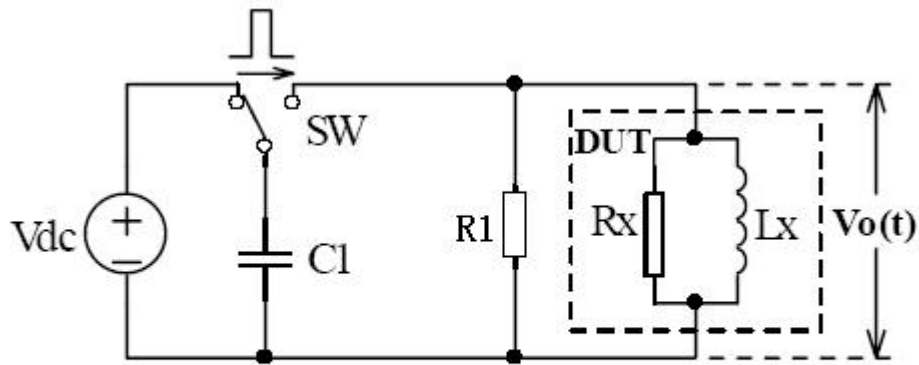



图 1-1 线圈脉冲测试原理简图

1-2

L

Q

L Q

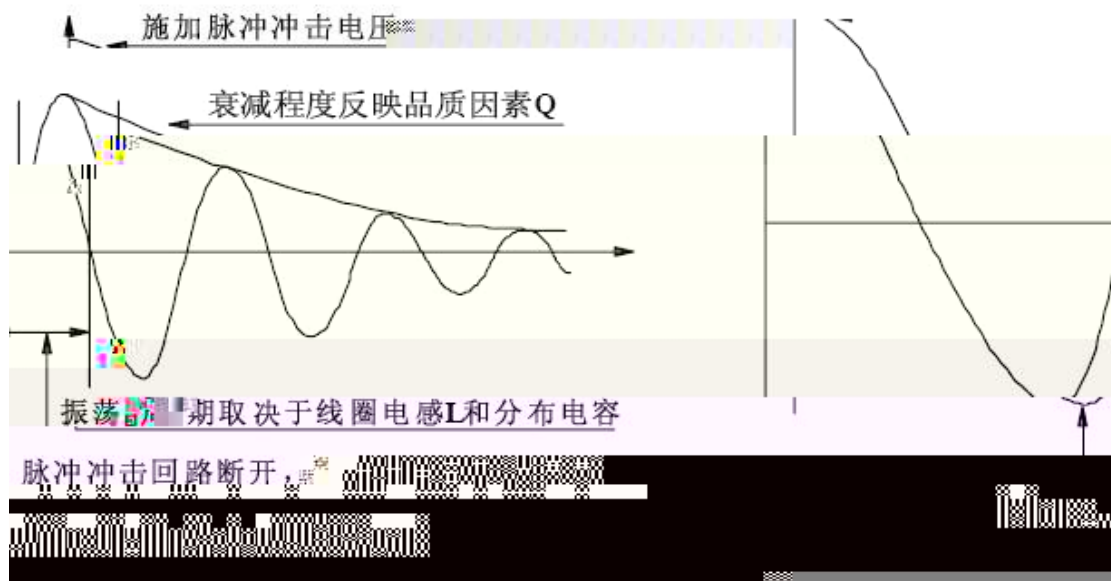

1



SCR

CRT()



20M

20uH

CRT

20mS

1mH

2



3

14		start stop power
----	--	------------------------

4.1

a)

b)

c)

d)

e)

f)

g)

h)

4.2

4.2.1

AB A B

a)

b)

c)

d)



HV	—
X	—→X
Y	—→Y
	—
	—

a)



c)

d)

e)

“ ”

f)

g)

h)

i)

e h

j)

4.3

4.3.1

4.3.2

1 $\varphi()$

U

V

U

V

2 Y

Y

U-W

V-W

U-W


V-W


3 Δ

Δ
 U-W
 V-U U-W V-U


4

H1 H2

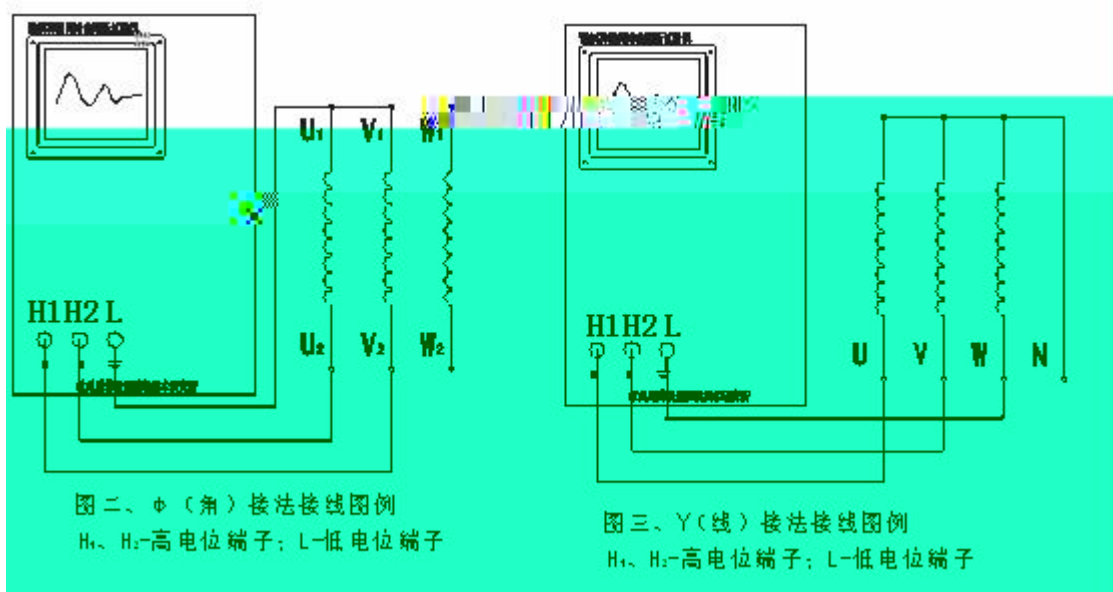

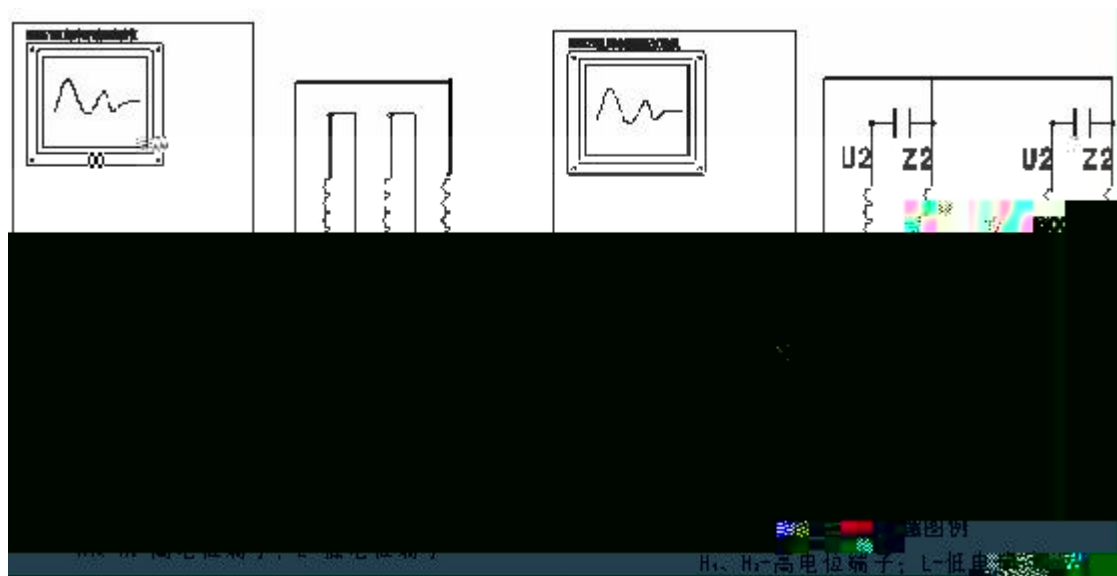

4.4

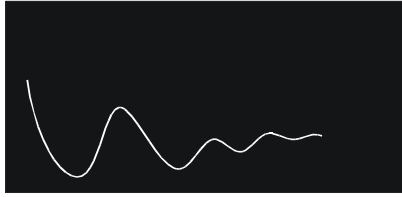

4.2

			H1	H2	L		
Y	1	1	U	V	W		
		2	V	W	U		W
			U	W	V		
	2	1	U	V	W		
		2	V	W	U		U
			U	W	V		V
	3	1	U	V	W		
		2	V	W	U		
			U	W	V		
		3	U	W	V		V
			V	W	U		U

4.3

			H1	H2	L		
Δ	1	1	U	V	W		
		2	U	W	V		UV
			V	W	U		
	2	1	U	V	W		
		2	U	W	V		WU
			V	W	U		
		3	U	W	V		WU
	3	1	U	V	W		
		2	U	W	V		
			V	W	U		VU
		3	V	W	U		VU

1

?

2

6.1

- 1. 19200
- 2. 8
- 3. 1
- 4.

6.2

()

--	--	--	--

7

		0x01	0x00	0x00	0x00	
--	--	------	------	------	------	--

603

		300	300	
--	--	-----	-----	--

- 1. 0xAA,
- 2.
- 3. 4
- 4. X Y
- 5.

6.3

0x01	
0x28	

